

# An educational setup for a laser induced breakdown spectroscopy (LIBS) system and its usage for the characterization of cultural heritage objects

Ioannis Sianoudis<sup>1</sup>, Anna Hein<sup>3</sup>, Giorgos Mitsou<sup>1</sup>, Maria Chatzidakis<sup>2</sup> and Eleni Drakaki<sup>4</sup>

<sup>1</sup>. Department of Physics, Chemistry & Materials Technology, Technological Educational Institute (TEI) of Athens, Ag. Spyridonas, 12210 Egaleo, Greece, jansian@teiath.gr, gmitsou@teiath.gr

<sup>2</sup>. TEI of Athens, Dep. of Conservation of Antiquities & Works of Art, maria\_chatzidakis@yahoo.gr

<sup>3</sup>. Institute of Materials Science, N.C.S.R. Demokritos, Greece hein@ims.demokritos.gr

<sup>4</sup>. Department of Physics, National Technical University of Athens, Zografou Campus, Athens 157 20, Greece, edrakaki@gmail.com

## Abstract

An experimental setup for laser induced breakdown spectroscopy (LIBS) has been developed for educational purposes, to be used in the physics curriculum of science students and of students who are specializing in the field of cultural heritage. The setup comprises basically a Q-switched Nd:YAG laser and a fiber optic spectrometer. All components were already existing equipment at the physics laboratories at the TEI of Athens, so that they could be assembled in-house to a considerably economic LIBS setup. The proposed laboratory exercises are focused on one hand on imparting the knowledge about physical principles and phenomena associated with the creation of plasma and the radiation processes. On the other hand the students will be trained in the operation and handling the actual analytical process, in terms of specific applications. Various parameters are examined, concerning the laser-matter interaction and the process issues, such as calibration, interpretation of spectra and evaluation of results. Exemplary measurements as an autonomous learning and teaching module were implemented, demonstrating the qualitative and quantitative analysis of various materials typically associated with cultural heritage objects, such as metal standards and original objects and replicas of mural paintings.

## Experimental setup

The experimental setup was implemented by assembling existing components. It is based on a Q-switched Nd:YAG laser, an optical system for focusing the beam and collecting the signal from the sample and a spectrometer. The timing and delay of the measurement, after each pulse of the laser, is controlled by a delay generator, which is inserted between the Q-switch unit and the spectrometer. This allows for setting different delay times for triggering the spectrometer. Figure 1 presents three photographs of the setup, while the schematically connection of the individual components is presented in Figure 2.

The laser (QuantaL, Brilliant B) exhibits a beam energy of 850 mJ and a pulse duration and frequency of 5μs and 10 Hz respectively. The 9 mm diameter beam is focused through a high power, planar convex lens with focal length f = 50 mm on the sample surface. In order to degrade the high energy density, a neutral filter with 10% transmission is inserted between laser and lens. The plasma light produced by the laser pulse is measured with a compact CCD spectrometer (HR2000, Ocean Optics), which is coupled with the optical fiber cable transmitting the plasma light from the target position.

The examined sample is placed on a mechanical x-y moving table. The exact position of the target point on the sample surface, i.e. the focus of the laser pulse, is controlled with a HeNe laser, the beam of which follows the axis of the excitation beam.

The delay generator, commonly used as trigger in most LIBS system, was replaced by a delay module (figure 3) that has been developed in house as a cheap and affordable solution for triggering. The trigger delay module is based on a Propeller microcontroller board (Parallax®) clocked at 80MHz. The task is to detect the Q-switch laser trigger pulse and to generate a delayed trigger pulse for the spectrometer. In order to minimize the response time the controller is programmed in low level language (Propeller Assembly). In this way the delay time can be software controlled in steps of 0.012μs with a minimum delay of 330 ns.

For acquiring and preliminarily processing the spectra the software Spectra Suite from Ocean Optics was used. For the peak assignment and the graphic presentation a demo version of Plasus - SpecLine and the software Origin, respectively, have been utilized.

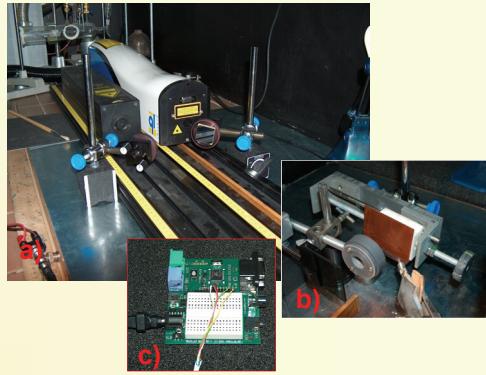
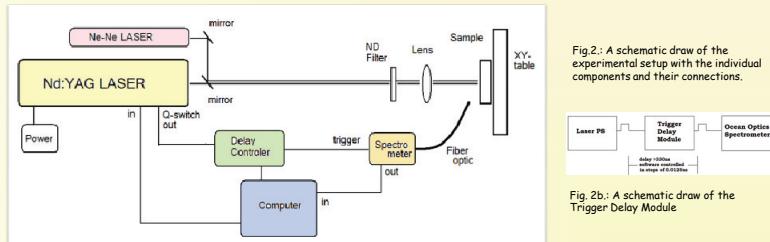


Fig. 1.: Photos of the experimental setup: a) the Laser systems, Nd:YAG and HeNe, on the optic table, b) the sample on the moving table with the focusing lens and the filter, c) the time delay module.

## Measurements and Results

The first part of the experiments is focused on testing the setup in terms of LIBS measurement parameters:

- a) **Calibration:** The spectra are evaluated qualitatively, i.e. through calibration of the energy/wavelength axis. Therefore the peaks are identified according to the matching spectral lines of the elements provided by the NIST Atomic Spectra Database. For this reason the demo software Plasus is applied (Fig. 3).
- b) **Effect of time delay:** The effect of the delay time of the trigger as an important parameter on the spectrum evaluation process is demonstrated in terms of recording evaluable spectra and in terms of controlling the spectrum quality. In Figure 4 a series spectra is presented obtained by changing gradually the delay time. While the intensity of the spectral lines is reduced, the spectral resolution is improved, as a consequence of the cooling of the plasma and the emission radiation originating from atoms and molecules. As optimum value a delay time of 4-5 μs was found.
- c) **Influence of laser beam energy:** In order to examine the effect of laser beam energy on the spectrum quality a series of spectra are recorded using different laser energies. For this reason various neutral filter with different transmission are applied. Figure 5 demonstrates the dependence of the line intensities on the pulse energy.


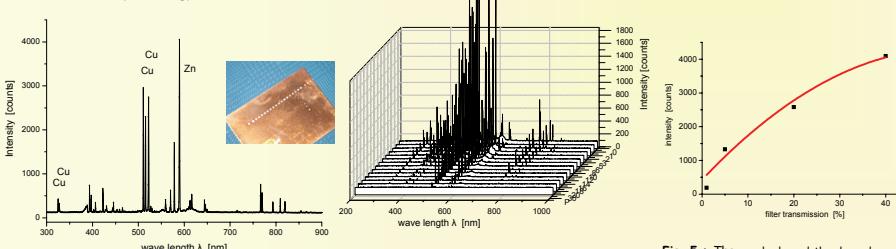


Fig. 5.: The graph showed the dependence of a Cu-line intensity from the beam energy of the Laser, expressed in transmission % of the used filter, as measured in spectra from a copper alloys sample obtained by a single pulse excitation,

## LIBS applications on cultural heritage objects

Analytical examination has become an integral part of the study and conservation of cultural heritage objects in terms of material characterization and in terms of monitoring deterioration processes. For this reason, students who are educated in this field, such as in archaeological science or in conservation science, have to pass commonly theoretical and practical training concerning the possibilities and limits of various analytical methods. Even though LIBS is not absolutely non-destructive the actual damage to the object remains considerably small and is compensated by advantages, such as the immediate spectrum generation, the portability and the absence of absorption effects for light elements in contrast to methods like XRF [1]. Therefore LIBS is applied both as complementary technique and as stand alone technique, particularly in the analysis of ancient metal objects and of pigments [2].

In collaboration with the Department of Conservation at the TEI of Athens a series of sample applications were developed demonstrating the principles of LIBS. Figure 6 illustrates the analysis of a metal object, which was recovered from the 'Patris' shipwreck and which was examined in view of the suitable corrosion treatment. The same object has been already analyzed with X-ray fluorescence (XRF) [3], indicating the elemental composition of the alloy. On the basis of the XRF spectrum the lines in the LIBS spectrum could be identified, revealing additionally the presence of light elements, which could not be detected with XRF, due to the absorption low energy X-rays in the air environment. Figure 7 presents a series of spectra acquired in measurements of replicas of mural paintings, representing the substrate and pigments from a typical palette from the Byzantine Period. Finally the feasibility of quantitative analysis is demonstrated with measurements of modern coins the elemental composition of which is known (Figure 8).

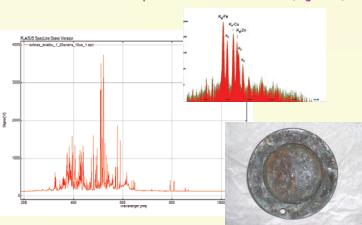


Fig. 6: A LIBS spectrum of a fragment of a pipe recovered from the 'Patris' shipwreck. In the inserts are shown the XRF spectrum and a photo of the pipe fragment respectively.

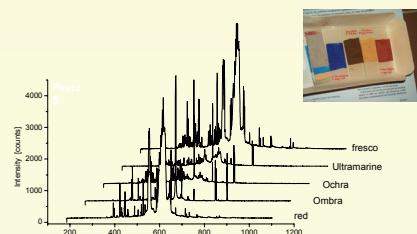


Fig. 7.: A series of LIBS spectra of Spectra of the wall painting pigments red, Ombré, Ochre, Ultramarine and the substrate fresco, as showed in insert photo.

## Conclusions

A setup of a Laser Induced Breakdown Spectroscopy (LIBS) system has been developed in order to be used for educational purposes. The LIBS setup was composed of a laser and low cost spectroscopy devices, which were available in the physics laboratory at the TEI of Athens. It was configured for the realization of a number of familiar and conventional laboratory exercises, such as obtaining atomic emission spectra or qualitative evaluation of the spectra. Furthermore the influence of several operational parameters on the spectrum quality was studied, such as the energy density of the laser beam, the time delay for triggering the spectrometer or the focal length of the used lens. The assembled LIBS setup was successfully tested in terms of the proposed experiments and it is expected to constitute a helpful educational package for laboratory exercises of students in physical sciences. Apart from teaching the scientific and technical aspects of LIBS, the system can be used as well for the education of students, who are trained in the field of Cultural Heritage, such as in archaeological science or in conservation science. These applications were demonstrated with a series of measurements focusing on the material characterization of metal objects and pigment layers.

## LIBS fundamentals

In LIBS, a high power laser pulse is focused onto the surface of the sample. Enough energy is delivered to a small volume to not only vaporize the material but to break all chemical bonds and ionize the elements present creating a small plasma plume. As the species in the plasma relax they emit at a characteristic wavelength. The spectrum evolves over time, becoming more distinct after several micro seconds. From this emission spectrum the constituent elements of the sample can be determined.

For the first few hundred ns after ablation the spectrum is dominated by continuum emission. Electron ion collisions in the plasma plume produce bremsstrahlung radiation across the bandwidth. Only the strongest elemental spectral lines can be observed over this background. As the plasma plume grows, the electron density of the plasma decreases and the continuum emission fades. After approximately 10 μs the spectral lines are clear enough to detect elements. The spectrometer needs to be able to gate the emission spectrum so that the early measurements can be disregarded. As the plasma plume expands, constituent atoms in the ionized gas become excited. Over just a few μs, the excited atoms began to relax, resulting in characteristic spectral emissions.

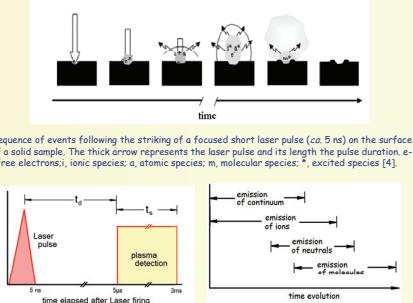


Fig. 8.: A print screen of the program SpectraSuite, where shows indicative spectra taken from measurements at a number of new Greek coins, Drachmas, as shown in inserted photo.

## References

- Giakoumaki A., Melassopoulaki K., Angelis D. Laser-induced breakdown spectroscopy (LIBS) in archaeological science—applications and prospects. *Anal Bioanal Chem* (2007) 387:749–760. 2007
- Bassisiotis, A., Diamantopoulou, A., Giannoudakis, F., Rouhani-Kalantzopoulou, M., Komitsas, Effects of experimental parameters in quantitative analysis of steel alloy by laser-induced breakdown spectroscopy. *Spectrochim Acta Part B* 56 (2001) 671-681.
- Sianoudis, I., Hein, A., Chatzidakis, M., Drakaki, E. and Hein, A. Educational LIBS experiments and XRF measurements with a portable setup adapted for the characterization of cultural heritage objects, *European Journal of Physics*, in press 2010.
- Celio Pasquini, Julian Cortez, Lucas M. C. Silva and Fabiano B. Gonzaga, Laser Induced Breakdown Spectroscopy, *J. Braz. Chem. Soc.*, Vol. 18, No. 3, 463-512, 2007